

Among the several adaptable preparation procedures, only two have been tested in this study: in lack of specific laws in force or standardised methods, self done testing undertaken by laboratories are not only "lawful", but also in conformity with the contents of the Circular 4/2000.

As regards methods repeatability, comparable and numerically rather low DS can be associated to the results obtained from both procedures. It can be observed that following the "wet" preparation a more homogeneous fibre distribution can be obtained, as results from low magnification analysis (125 X). These samples are more suitable for the analysis because the fibres are not clumped, but they're well distributed on the filter.

The results obtained using both the ECB and the Italian Circular 4/2000 protocols aren't too different. The ECB method doesn't need the determination of fibres length: that's why, according to the adopted procedures, the characterisation may be carried out without evaluating fibres length.

The described work in progress is leading to the drawing up on a CONTARP internal protocol for risk assessment related to the managing of MMVF.

Moreover, it will be possible to assess the accuracy of the results through the statistical treatment of the data.

[1] International Agency For Research On Cancer. *IARC Monographs On The Evaluation Of The Carcinogenic Risk Of Chemicals To Humans*, 81 (2002).

[2] Decreto del Ministero della Sanità 1 Settembre 1998. *G.U. 271* (1998).

[3] Circolare del Ministero della Sanità N. 4. *G.U. 88* (2000).

[4] European Chemical Bureau. *ECB/TM/1(00) rev 2, Draft-4*, (2000).

[5] Marconi A., Chiamonte C., Castellet Y Ballarà G., Cacchioli E. *SYMPOSIA: I CONGRESSI DELLA FONDAZIONE MAUGERI*, 4: 185-190 (2000).

[6] Marconi A., Castellet Y Ballarà G., Cacchioli E., Fizzano M. R., Camillucci L., Campopiano A., De Blasi P. *ATTI 19° CONGRESSO NAZIONALE AIDII: 70-74* (2001).

[7] Incocciati E., Massera S., Nappi F., Barreca F. *ATTI 22° CONGRESSO NAZIONALE AIDII*, 175-178 (2004).

[8] Bacci T., Sala O., Renna E., Pecchini G., FERDENZI P. *ATTI 22° CONGRESSO NAZIONALE AIDII*, 184-187 (2004).

[9] DECRETO LEGISLATIVO N. 277 in Supp. Ord. G.U. n. 200 (1991).

## ANALYTICAL EVALUATION OF WASTES CONTAINING ASBESTOS AFTER INERTIZATION TREATMENT BY PYROLITIC PROCESS

**Giovanni Pecchini<sup>(1)</sup>, Alessandro F. Gualtieri<sup>(2)</sup>, Emilio.Renna<sup>(1)</sup>, Orietta.Sala<sup>(1)</sup>, Luigi Calzavacca<sup>(3)</sup>, Tiziana Bacci<sup>(1)</sup>, Federica Paoli<sup>(1)</sup>, Valeria Biancolini<sup>(1)</sup>**

<sup>(1)</sup>ARPA, Sezione Provinciale di Reggio Emilia

<sup>(2)</sup>Dipartimento di Scienze della Terra, Università degli Studi di Modena e Reggio Emilia.

<sup>(3)</sup>Eco Studio - Aspireco, Gavardo Brescia

Wastes recovery efficiency have been slightly improved by Decree n.248 of 29/7/2004 on "Rules on determination and disciplines of recovery activities of products and goods of asbestos and containing asbestos" by defining processes and treatment able to bring to a complete transformation of crystallochemical features of asbestos.

Such treatments if properly applied allows to avoid the disposal of wastes in dumps. They also allow the reutilization of processed wastes. No adequate power plants suitable for the mentioned treatment presently exist in Italy.

Intense research activity is devoted to the start up of pyrolitic processes applied to wastes deriving from concrete/asbestos to be reutilized in environmental recovery. Decree n.248 reports characteristics of processed material which must be asbestos free and accompanied by mineralogical composition of final product.

Present paper propose an analytical protocol suitable for law need and able to guarantee safety conditions of wastes after crystallochemical transformation.

In order to verify such transformations analytical procedures adopted in qualified laboratories on asbestos analysis have been utilized. Pure chrysotile and concrete/asbestos samples have been analyzed by MOCF, DRX, SEM and FTIR after 2 hours heating at 600-700-800-900-1000 °C in muffle furnace. Some samples processed by pilot power plant by Aspireco have also been analyzed.

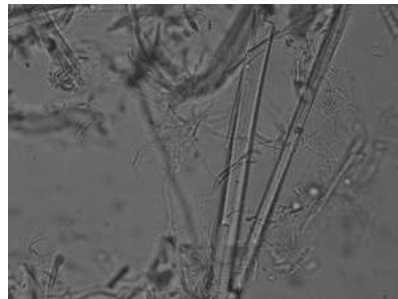
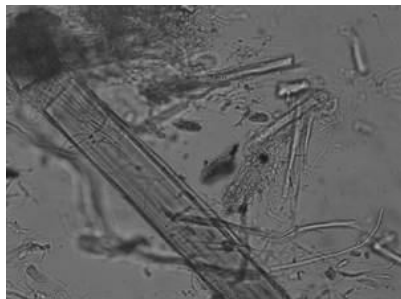


Figure 1-2. Chrysotile sample after pyrolitic treatment in pilot power plant.

Main high temperature transformations of asbestos containing materials are described as solid state deoxydrilization and recrystallizations (Gualtieri and Tartaglia, 2000). Thermal treatment of pure chrysotile evidences that after deoxydrilization at 800 °C starts a solid state transformation which brings to a complete recrystallization into silicatic-magnesiatic phases (forsterite and enstatite). After this transformation chrysotile loses fiber-asbestos characteristic and is not dangerous for health. Asbestos by pure tremolitic amphibole thermally processed at 1100 °C after deoxydrilization is completely transformed in diopside, enstatite and cristobalite. Flaked asbestos represented by chrysotile and processed at 1000 °C show that asbestos original characteristic is completely decomposed and three new phases of gehlenite, diopside and iron forsterite are cristallized. X ray diffractometry of concrete/asbestos constituted by prevailing chrysotile processed at 1100 °C evidence new phases deriving from chrysotile transformation such as prevailing gehlenite and diopside in a less extent. Quartz and hematite have also been found as residuals. SEM analysis of obtained materials evidence the inertization of fibrous phases which are transformed into irregular aggregates of neoformation crystals accompanied by loss of original dangerous character.

#### MOLP

Is the simplest technique which enables to verify optical properties of asbestos crystals.

Chrysotile processed at relatively low temperatures (600-700 °C) is still characterized by original colour and colour changes which completely disappear at higher temperatures evidencing the complete crystalline structure transformation.

#### DRX


Main (12.1°) and secondary (24.3°) reflexed rays expressed as 2 Theta are recognizable on chrysotile and concrete/asbestos samples processed at 600-700 °C while are not visible on samples processed at temperatures higher than 800 °C. A detailed study on diffractogram allows to recognize new recrystallization phases.

#### SEM

Chrysotile fibers morphology tends to modify loosing characteristic flexuous curves of chrysotile and assuming a rigid character closer to artificial mineral fibers. New recrystallized fibers tend to broke transversally differently to asbestos ones. Qualitative analysis of EDX spectra evidences an increasing oxygen loss related to increasing temperature of the sample.

#### FTIR

FT-IR spectrophotometry is a highly sensitive analytical method which allows to analyze samples in relatively short times and good repetivity. Samples of KBr, chrysotile and concrete/asbestos have been grinded , transformed into tablets and analyzed. A decreasing of characteristic peak in chrysotile spectra related to increasing processing temperature was detected. The peak completely disappeared on samples processed at temperatures higher than 800 °C evidencing the complete transformation of chrysotile.

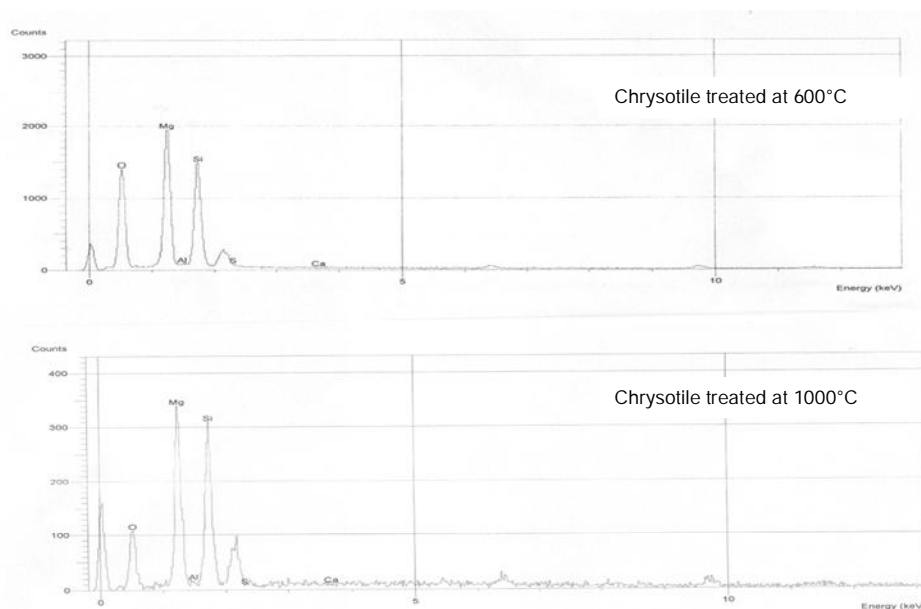

In conclusion the contemporary study of the same samples with all listed methods allows sure diagnosis on processed wastes.

#### References

Gualtieri A.F., Tartaglia A. (2000) Thermal decomposition of asbestos and recycling in traditional ceramics. Journal of the European Ceramic Society. 20 (9), 1409-1418.